# Monitor setup and software for the T4 Science hydrogen maser 66

P. de Vicente, R. Bolaño, L. Barbas

Informe Técnico IT-OAN 2011-5

# Revision history

| Version | Date | Author | Updates |
|---|---|---|---|
| 1.0 | 10-03-2011 | P. de Vicente | First version |

# Contents

**1 Introduction** **3**

**2 An overview on the installation** **3**

**3 Assigning an IP address** **4**

**4 Measuring the drift** **5**
4.1 Code in Linux: Daemon . . . . . 5

**5 Tuning the maser. Remote control** **8**

**6 Comparison between both masers** **11**

**7 Database and web interface** **13**

# 1 Introduction

A new hydrogen maser was purchased from T4-Science and installed in Yebes in February 22nd, 2011. The model is iMaser EFOS C, Serial Number: 66. We describe the works performed to monitor the maser and tune it.

# 2 An overview on the installation

The hydrogen maser was installed in february 22nd 2011 in the maser room located in the basement of the 40 m tower building besides EFOS Serial Number 37. In order to distinguish between both of them we will refer to the new one by imaser66 and to the rented one by imaser37 respectively.

Image 1 shows a picture of the new clock in the room.

Figure 1: *EFOS Maser S/N 66 in its room. Battery at the bottom.*

Imaser 66 is similar to imaser37, but its remote control and monitor is done via an ethernet port. The ethernet port is implemented with an internal serial to ethernet card. There are other minimal differences related to the diagnostic LEDs on the back of the maser. The maser rack stands on 4 legs with suspension which prevent vibrations from the floor affecting the equipment.

Currently two signals are sent to the backends room using RG-144 cables: 5 MHz and 1 PPS.

T4 Science provides an account in its FTP server with three areas: one for documentation which contains three manuals, and the other two to upload data from maser 37 and 66

respectively. The software management has been written according to the specifications and information provided in the manuals.

# 3 Assigning an IP address

Imaser 66 has got an embedded PC with an ethernet port and at least one serial port inside The model is a NetDCU8 which uses a Samsung ARM9 processor running Windows CE. In order to monitor the maser we changed its IP address to match our VLAN. The best way is to use a switch to which the maser and a laptop with Linux is connected. The Linux PC ethernet port should be setup with an IP address in the same LAN as the maser. The original IP address for the maser is 10.7.114.8.

A telnet sessino is opened from the laptop. The embedded PC will ask for a username and a password. Neither the Username nor the password are provided in this report to prevent being compromised but can be found them in the maser notebook. From the telnet session we should type some commands. Below we include the log of a session. Commands are those typed after the prompt: !>

```
\>cd Windows
\Windows>ndcucfg

NetDCU Config Utility Ready
Version: 033
Type help for commands

!>reg open \comm\dm9ce1\parms\tcpip
OK
!>reg enum
OK -> reg enum key \
OK -> reg enum value \
   00 "defaultgateway"=string:10.7.114.1 \
   01 "ipaddress"=string:10.7.114.8 \
   02 "DNS"0string:195.186.1.162 \
   03 "subnetmask"=string.255.255.255.0 \
   04 "EnableDHCP"=dword:0 \
   05 "UseZeroBroadcast"=dword:0 \
OK
!>reg set value defaultgateway string 192.168.0.1
OK
OK
!>reg set value ipaddress string 192.168.0.197
OK
OK
!>reg set value DNS string 192.168.0.1
OK
OK
!>reg set value subnetmask string 255.255.255.0
```

```
OK
OK
!>reg save
OK
!>reboot hardware
```

Afterwards the maser will be reachable in IP address 192.168.0.197.

# 4 Measuring the drift

In order to tune the frequency of the maser we measured its drift. As with other masers, the drift is obtained by comparing 1 PPS from the maser and 1 PPS from the GPS for a long time interval. Due to the lack of an external timing box, the 1 PPS from the maser is generated inside the maser, unlike with imaser37 where we use the VLBI data acquisition Time Box. Both pulses are compared by an HP 53131A counter with 1 ps accuracy. For the time being we are using an HP 53132 counter from the lab. Two new counters are expected to arrive during 2011.

The new counter is managed remotely via a GPIB port. The 53132 counter has been connected to the same bus as the 53131A in the GPIB PCI card of host "meteomaser", with GPIB address 3. The new counter works with a 5 MHz frequency reference from imaser 37.

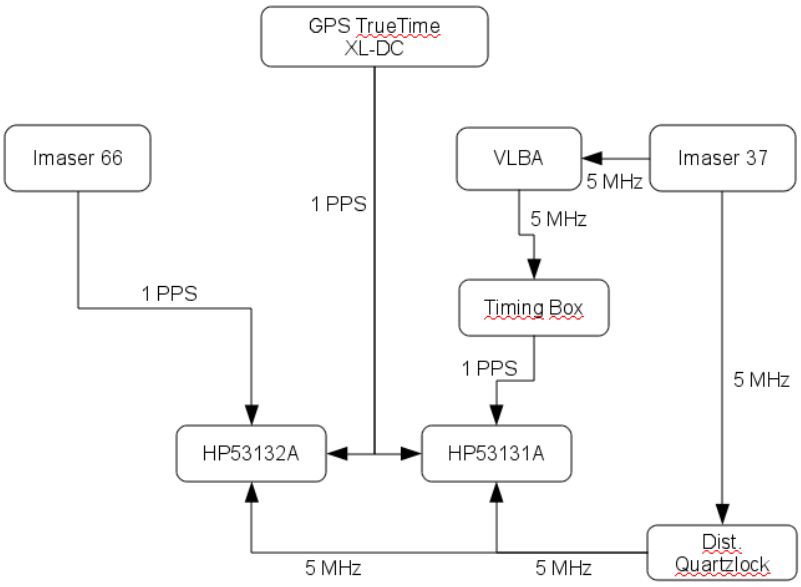


Figure 2: *Setup to monitor the relative frequency error of both masers compared to the GPS.*

## 4.1 Code in Linux: Daemon

The comparison between 1 PPS from the GPS and 1 PPS from the maser is done by the counter after an initialization sequence which sets each counter. This initialization is governed by a

program running as a daemon in a devoted Linux PC. The daemon starts during the PC boot sequence. The daemon has been modified to control two different counters at the same time. Each counter is managed by a different instance of a single C++ class which allows to control HP 53131A/53132 counters. These two instances are created at the beginning of the Daemon. Below we show how this is acomplished:

```
HPcounter * counter_im37;
HPcounter * counter_im66;


try {
   counter_im37 = new HPcounter(0,4);
   counter_im37->setModeComparator(1.3,1.3);
   im37OK = true;
} catch (HPcounter::HPcounterException & s){
   if (DEBUG)
       printf("Excepcion: %s, Ibsta: %d, Iberr: %d\n", s.ShowMsg(), s.ShowStat(), s.ShowErr());
       im37OK = false;
}

try {
   counter_im66 = new HPcounter(0,3);
   counter_im66->setModeComparator(1.3,1.3);
   im66OK = true;
} catch (HPcounter::HPcounterException & s){
   if (DEBUG)
      printf("Excepcion: %s, Ibsta: %d, Iberr: %d\n", s.ShowMsg(), s.ShowStat(), s.ShowErr());
      im66OK = false;
}
```

The constructor of the `HPcounter` class accepts the board address (always 0) and the GPIB address of the device (4 for imaser37 counter and 3 for imaser66 counter). It resets the counter by sending the following SCPI messages:

```
writeToHP("*RST");
writeToHP("*CLS");
writeToHP("*SRE 0");
writeToHP("*ESE 0");
writeToHP(":STAT:PRES");
```

Method `setModeComparator()` sets the counters to measure the time interval between both 1 PPS signals:

```
writeToHP(":CONF:TINT");
writeToHP("FUNC 'TINT'");
// We switch off the levels
writeToHP(":EVEN:LEV:AUTO OFF");
// Signal in channel 1
// Manually set the levels of trigger.
sprintf(instr, ":EVEN:LEV %f V", lev1);
writeToHP(instr);
// Positive slope for the trigger
writeToHP(":EVEN:SLOP POS");
// Impedance of the signal: 50 Ohms
writeToHP(":INP:IMP 50");
writeToHP(":INP:COUP DC");
writeToHP(":INP:ATT 1");
writeToHP(":INP:FILT OFF");
writeToHP(":EVEN:HYST:REL 0");

// Signal in channel 1
// Manually set the levels of trigger.
writeToHP(":EVEN2:LEV:AUTO OFF");
sprintf(instr, ":EVEN2:LEV %f V", lev2);
```

```
writeToHP(instr);
// Positive slope for the trigger
writeToHP(":EVEN2:SLOP POS");
// Impedance of the signal: 50 Ohms
writeToHP(":INP2:IMP 50");
writeToHP(":INP2:COUP DC");
writeToHP(":INP2:ATT 1");
writeToHP(":INP2:FILT OFF");
writeToHP(":EVEN2:HYST:REL 0");
```

The daemon then starts an infinite loop which reads both counters, and after each measuremnt processes the data. Each cycle of the loop takes 2 seconds to complete. The counter reads the time interval with the following instructions:

```
writeToHP(":INIT:CONT ON");
writeToHP(":FETCH:TINT?");
readFromHP(data);
```

where `writeToHP()` and `readFromHP()` are high level calls to write and read in the GPIB port.

The processing of the data is as follows:

- Each individual value is stored in a local variable and written on an intermediate file `data10m.log` with two columns, one per counter.
- Each individual value is also stored in a shared memory variable, available to third part applications.
- Every ten minutes the function reads file `data10m.log`, computes the mean value and RMS of the time difference between the pulses and resets the file.
- The mean value and the RMS for both masers are stored in shared memory variables and written on a database. The database contains two tables, one per maser and counter.

Shared memory variables are defined and reserved in a structure which is defined via a program called `get_countermem` which is run during the PC startup. The structure is the following:

```
struct maserdata {
 double modifiedJulianDay;
 double gps_im37_diff;
 double gps_im37_diff_10m;
 double gps_im37_rms_10m;
 double modifiedJulianDay_im66;
 double gps_im66_diff;
 double gps_im66_diff_10m;
 double gps_im66_rms_10m;
};
struct maserdata * shm_maserdata;
```

Variables `modifiedJulianDay` and `modifiedJulianDay_im66` are duplicated and contain the same values.

In order to find out the current values of the comparison the user, can run program `maserStatus` which produces the following output with instantaneous, mean and RMS values for both masers:

```
./maserStatus
*** Shared memory content ***
Modified Julian Day: 55656.6231  55656.6231
Offset (each 1 sec)
         im37:  915.40 ns
         im66: -926.10 ns
Average and rms (10 min)
         im37:  912.45 ns    0.00 ns
         im66: -926.95 ns    0.00 ns
```

These values are available from any ACS client by using the gpsMaserComparator component but only one of the masers is available at a time. In order to get the values from the other maser, file `GPS_MASER_COMP_1` in the CDB database should be modified with the correct serial number (either 37 or 66):

```
imaser="37"
```

# 5 Tuning the maser. Remote control

The maser control (and tuning) is done using a Python class with similar functionality to the one written for imaser 37. The new class, named `imaser66`, uses UDP sockets on port 14000. This version has some functionality not present in imaser37. It has some methods which allow to:

- `enableHTML(on)` Start to display the monitoring of the Maser on the HTML page.
- `recordData(interval)` Record the monitoring in a file stored on the local SD memory card. The time period can be selected. Whenever the file reaches 2 MB size it is copied to a second file with a name including the data and time. The first file is reset. We have found that the commanded interval time does not match the one used and differs several minutes from it.
- `enableSerial(on)` Stop the serial communication between the network module and the maser.
- `setDeltaFrequency(df)` Correct the frequency by providing the relative error in frequency. Unlike imaser37 no intermediate calculations are required.
- `getFrequency()` Get the maser frequency ($\simeq$ 1420 MHz).

More methods are available but we have not mentioned them here since they provide less used functionalities.

Class `imaser66` is used by two python programs: `correctiMaser66.py`, which corrects the frequency of the maser and `imaser66Status2DB.py` which writes the status information from the maser in a database. The status of the maser is composed of the list of parameters in table 1.

The status of the maser can be obtained with a periodicity of 5 seconds by using a web browser. Fig 3 is a snapshot of the web page.

`correctiMaser66.py` is a python script which corrects the frequency of the maser. It uses a class which contains two methods for getting information from the maser status. One retreives the data from the internal imaser FTP server. The data from this server is parsed and

| Channel | Description | Name | [physical unit/LSB] |
|---|---|---|---|
| 1 | Battery voltage A | U batt.A [V] | 2.441E-02 |
| 2 | Battery current A | I batt. A [A] | 1.221E-03 |
| 3 | Battery voltage B | U batt.B [V] | 2.441E-02 |
| 4 | Battery current B | I batt. B [A] | 1.221E-03 |
| 5 | Hydrogen pressure setting | Set. H [V] | 3.662E-03 |
| 6 | Hydrogen pressure measurement | Meas. H [V] | 1.221E-03 |
| 7 | Purifier current | I purifier [A] | 1.221E-03 |
| 8 | Dissociator current | I dissociator [A] | 1.221E-03 |
| 9 | Dissociator light | H light [V] | 1.221E-03 |
| 10 | Internal top heater | IT heater [V] | 4.883E-03 |
| 11 | Internal bottom heater | IB heater [V] | 4.883E-03 |
| 12 | Internal side heater | IS heater [V] | 4.883E-03 |
| 13 | Thermal control unit heater | UTC heater [V] | 4.883E-03 |
| 14 | External side heater | ES heater [V] | 4.883E-03 |
| 15 | External bottom heater | EB heater [V] | 4.883E-03 |
| 16 | Isolator heater | I heater [V] | 4.883E-03 |
| 17 | Tube heater | T heater [V] | 4.883E-03 |
| 18 | Boxes temperature | Boxes temp. [C] | 2.441E-02 |
| 19 | Boxes current | I Boxes [A] | 1.221E-03 |
| 20 | Ambient temperature | Amb. Temp. [C] | 1.221E-02 |
| 21 | C-field voltage | C field [V] | 2.441E-03 |
| 22 | Varactor voltage | U varactor [V] | 2.441E-03 |
| 23 | external high voltage value | U HT ext. [Kv] | 1.221E-03 |
| 24 | external high voltage current | I HT ext. [uA] | 1.221E-01 |
| 25 | internal high voltage value | U HT int. [kV] | 1.221E-03 |
| 26 | internal high voltage current | I HT int. [uA] | 1.221E-01 |
| 27 | Hydrogen storage pressure | Sto. press. [bar] | 4.883E-03 |
| 28 | Hydrogen storage heater | Sto. heater [V] | 6.104E-03 |
| 29 | Pirani heater | Pir. heater [V] | 6.104E-03 |
| 30 | Unused | Unused [] | 0.000E+00 |
| 31 | 405 kHz Amplitude | U 405 kHz [V] | 3.662E-03 |
| 32 | OCXO varicap voltage | U ocxo [V] | 2.441E-03 |
| 33 | +24 V supply voltage | +24Vdc [V] | 9.766E-02 |
| 34 | +15 V supply voltage | +15Vdc [V] | 7.813E-02 |
| 35 | -15 V supply voltage | -15Vdc [V] | -7.813E-02 |
| 36 | +5 V supply voltage | +5Vdc [V] | 3.906E-02 |
| 37 | -5 V supply voltage | -5Vdc [V] | -3.906E-02 |
| 38 | +8 V supply voltage | +8Vdc [V] | 3.906E-02 |
| 39 | +18 V supply voltage | +18Vdc [V] | 7.813E-02 |
| 40 | Unused | Unused [] | 0.000E+00 |

Table 1: *List of iMaser monitor parameters. Taken from the imaser manual*




| | | | | | |
|---|---|---|---|---|---|
| **U batt.A[V]** | 27.612 | **EB heater[V]** | 12.256 | **Pirani heat.[V]** | 12.042 |
| **I batt.A[A]** | 0.104 | **I heater[V]** | 7.246 | **Unused** | 0 |
| **U batt.B[V]** | 28.149 | **T heater[V]** | 9.429 | **U 405kHz[V]** | 11.3435 |
| **I batt.B[A]** | 3.085 | **Boxes temp[°C]** | 44.653 | **U OCXO[V]** | 5.271 |
| **Set H[V]** | 5.321 | **I boxes[A]** | 0.411 | **+24 VDC[V]** | 24.51 |
| **Meas. H[V]** | 1.273 | **Amb.temp.[°c]** | 21.533 | **+15 VDC[V]** | 14.38 |
| **I pur.[A]** | 0.442 | **C field[V]** | 5.315 | **-15 VDC[V]** | -15.39 |
| **I diss.[A]** | 0.387 | **U varactor[V]** | 4.648 | **+5 VDC[V]** | 5.04 |
| **H light[V]** | 4.514 | **U HT ext.[kV]** | 3.507 | **-5 VDC[V]** | 0 |
| **IT heater[V]** | 9.658 | **I HT ext[uA]** | 3.052 | **+8 VDC[V]** | 7.89 |
| **IB heater[V]** | 10.474 | **U HT int.[kV]** | 3.505 | **+18 VDC[V]** | 17.27 |
| **IS heater[V]** | 9.995 | **I HT int.[uA]** | 3.052 | **Unused** | 0 |
| **UTC heater[V]** | 12.598 | **H st.pres.[bar]** | 1.118 | **Lock** | 1 |
| **ES heater[V]** | 11.089 | **H st. heat[V]** | 14.075 | **DDS** | 1420405750.299098 |

Figure 3: *Web page with information from imaser66. The content is updated every 5 seconds.*

may be outdated as much as the time period of the FTP server. The second method obtains the data from the web server and parses the data there. The information is 5 seconds old at most since this web is refreshed with instantaneous values with a periodicity of 5 seconds. Below is an example on how to use the script:

```
./correctiMaser66.py 9.5e-13
Connecting to the maser ...
Do you want to see all current parameters y/[n]) ? y

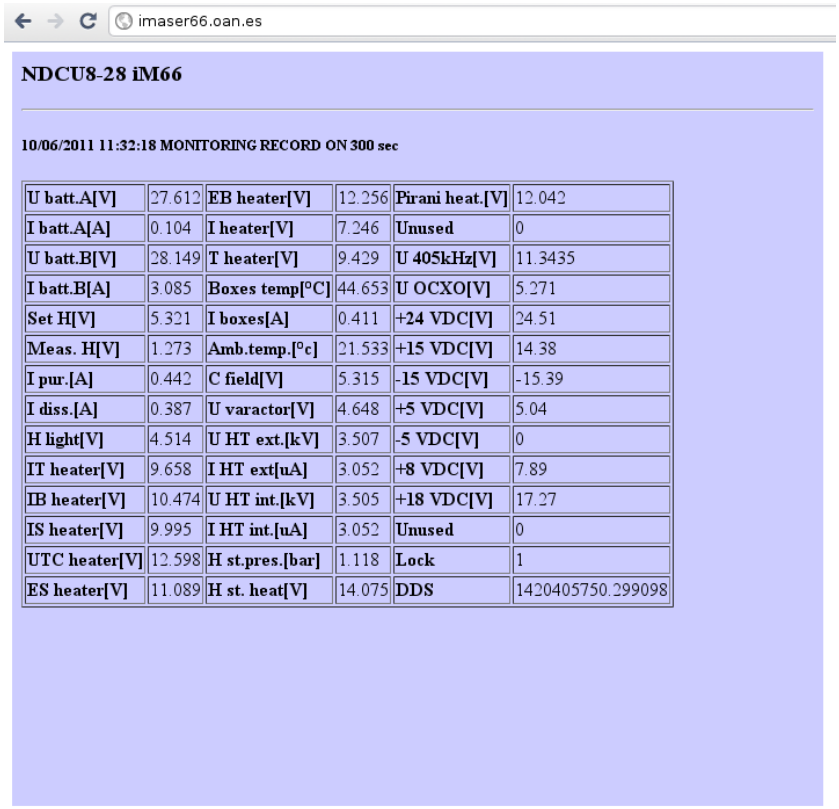[27.611999999999998, 0.10100000000000001, 28.149000000000001,  ....

1420405750.3

Current Maser frequency: 1420405750.297752  Hz
Do you want to apply this correction 9.5e-13 y/[n]) ? y
Applying the correction ...
Maser frequency after the correction: 1420405750.299098 Hz
```

One tuning was enough to acquire a relative frequency error below $10^{-13}$. The correction was done on 17/3/2011. Table 2 summarizes the date and time of the tuning, the measured drift and the correction applied. The measured drift ($-9.5\,10^{-13}$) was obtained from the slope of the graph and the negative sign indicates that the function is decreasing. The function represents the time elapsed between 1 PPS coming from the GPS and 1 PPS coming from the maser. If the function is negative it means that the maser ticks slower than the GPS and both pulses get more apart with time. In order to correct the maser frequency we had to command a positive value, that is, the relative frequency by which we want to increase maser frequency. According to the script the frequency of the maser before the tuning was 1420405750.297752 Hz and 1420405750.299098 Hz after the correction.

| Date | Time (UTC) | Meas. $\Delta f/f$ | Appl. $\Delta f/f$ |
|---|---|---|---|
| 17/03/2011 | 12:50 | $-9.5\,10^{-13}$ | $9.5\,10^{-13}$ |

Table 2: *Date and time of the tuning. The measured drift is the drift up to the tuning date. The correction was applied in that date and time.*

# 6 Comparison between both masers

We compared the plots for both masers (maser - GPS) during 7 days after taking out the long term drift for both individual graphs. The result can be seen in figure 5.

According to figure 5 we did not succeed in removing completely the long term drift. However it is very clear that the short term variations appear in both graphs with the same intensity. Since the only common element was the GPS (and the 5 MHz synchronization signal in the counters), we can conlude that these effects come from the GPS receiver. It is pobable that the weather and conditions in the atmosphere affect the signal from the satellites. At the end of the week we can see that there was jump downwards which is also common to both systems.

In order to check the difference between both masers we have substracted the data from both of them, during 7 days and plotted it, taking out the slope, which corresponds to the relative frequency difference between them. The resulting graph is rather awkward and is displayed in

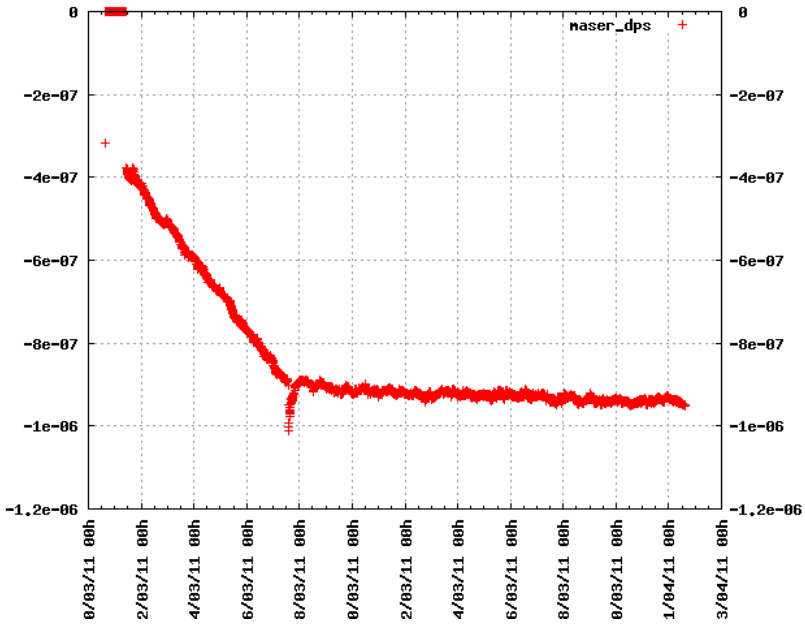


Figure 4: *Maser drift since installation to April 1st 2011. The time units are Modified Julian Days. Tuning was done on March 17th, 2011. The jump seen when tunning is due to an unknown origin and affected both masers, therefore it may come from the GPS receiver.*

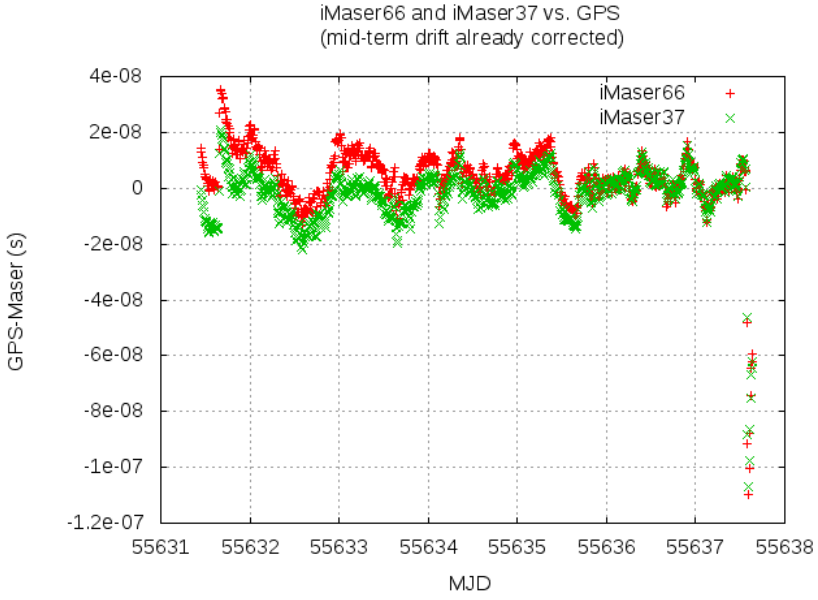


Figure 5: *Time ellapsed between the GPS 1 PPS and the maser 1 PPS for both masers during a week. The long term drift was substracted.*

figure 6. The data is a sort of square waveform with a period of 48 hours and an amplitude of 2 ns. This behaviour requires further investigation to know if this is a numeric effect coming from the data acquisition. To check if this behaviour is real and comes from one of the masers a new setup should be used, in which the 1 PPS from each maser are injected into one counter and the time difference between them recorded.

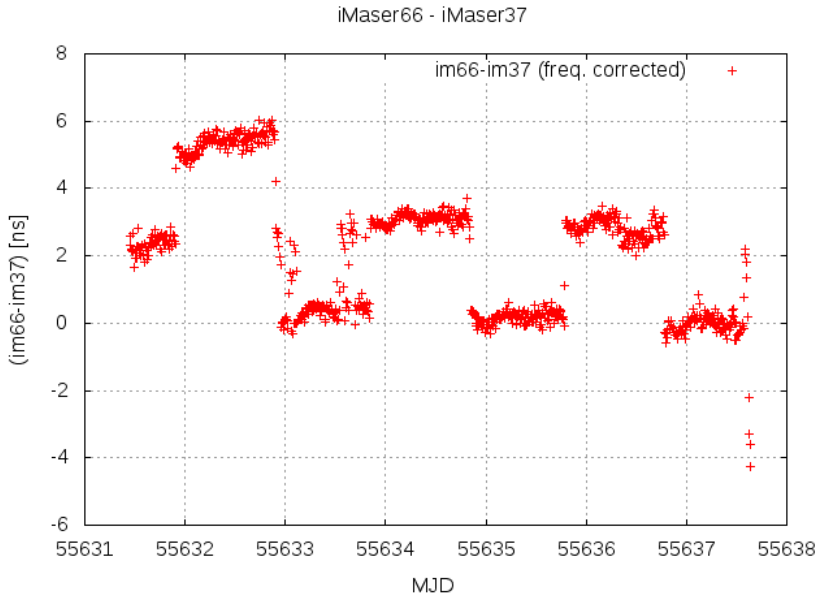


Figure 6: *Time difference between masers 66 and 37 after removing the long term drift which corresponds to the difference in frequency between both masers*

# 7 Database and web interface

The database was updated with two new tables for maser66: one containing the comparison with the GPS every 10 minutes and another one with the status of the maser. These tables have the same fields as the ones for maser 37 and can be queried from the same web application described in report OAN-2010-1.

Currently the database contains 7 tables: two per each maser that has worked in the Observatory, CH1-75 (Kvarz), imaser37 (T4Science) amd imaser66 (T4Science) and one that contains the room temperature up to 22-01-2009. The room temperature for the maser room is stored currently in a different database. Table 3 contains the dates since which we have data for the masers in Yebes.

A web interface located in `http://hera.oan.es/graficas_interactivas/` allows to plot the drift and different status variables of imasers 66 and 37 from the private OAN LAN. The maser to be used is chosen from the upper combo box. The lower combo box allows to select the parameter that we want to plot. Below are the date/time interval from a calendar widget, the plot title, axis labels, and the X axis resolution. The final plot is shown on a separate

| Maser | Start date (data) | Stop date (data) | Installation date | Stop working date |
|---|---|---|---|---|
| CH1-75 (data) | 01-10-1998 | 28-08-2009(*) | 04-12-1995 | 15-06-2009 |
| CH1-75 (status) | 04-12-1995 | 02-02-2009 | 04-12-1995 | 15-06-2009 |
| imaser37 (data) | 28-08-2009 | | 28-08-2009 | |
| imaser37 (status) | 16-09-2009 | | 28-08-2009 | |
| imaser66 (data) | 10-03-2011 | | 22-02-2011 | |
| imaser66 (status) | 24-03-2011 | | 22-02-2011 | |

Table 3: *Date ranges for which the database have stored data from the masers in Yebes. (*) The CH1-75 worked correctly until 15-06-2009.*

tab in the browser. Data can also be extracted and stored in an ASCII local file with two columns: date and value.

Figure 7 shows a snapshot of the web page that allows to plot any of the previous maser parameters as a function of time and where both maser tables can be selectable.

# References

[Vicente & Garrigues 2005] P. de Vicente, A. Garrigues. "Monitorización del máser de hidrógeno del CAY", IT–OAN 2005-5

[Vicente et al. 2007] P. de Vicente, J.D. Gallego, R. Bolano, C. Almendros. "Monitorización del máser de hidrógeno antes y después del traslado al radiotelescopio de 40m", IT–OAN 2007-3

[Vicente2010] P. de Vicente, S. García-Espada, A. Barcia, R. Bolaño, L. Barbas. "Tuning the T4 Science hydrogen maser" IT-OAN 2010-1

[T4Science, 2008] T4 Science SA. "Installation, Operation and Maintenance User Manual", 2008

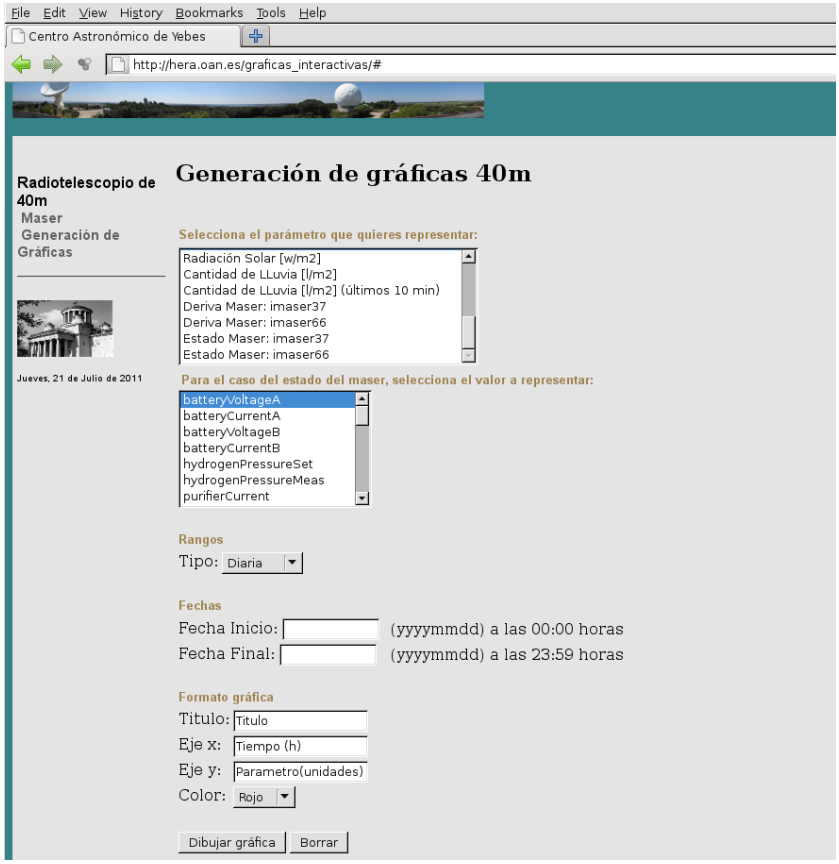


Figure 7: *Web page at http://hera.oan.es/graficas_interactivas/ which allows to plot maser parameters as a function of time. The upper combo box allows to select any of the two tables (data and status) from imaser 37 and 66.*